

FIG. 1


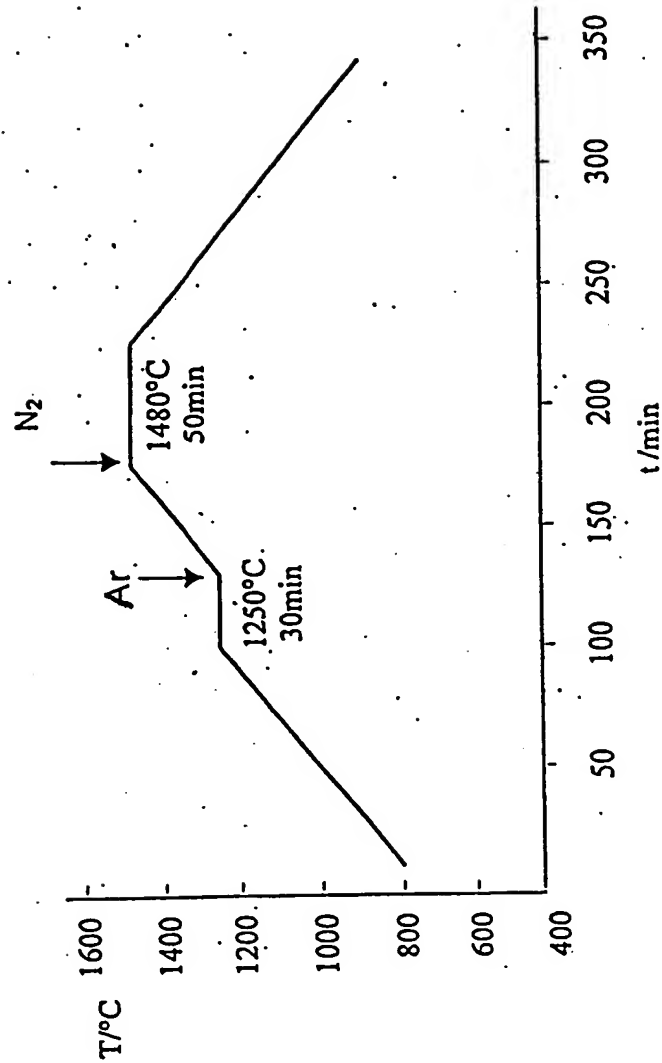


FIG. 2a

Tiefenprofil-Massen% DEPTH PROFILE MASS%  
SAMPLE A Vacuum


Probe A-Vakuum

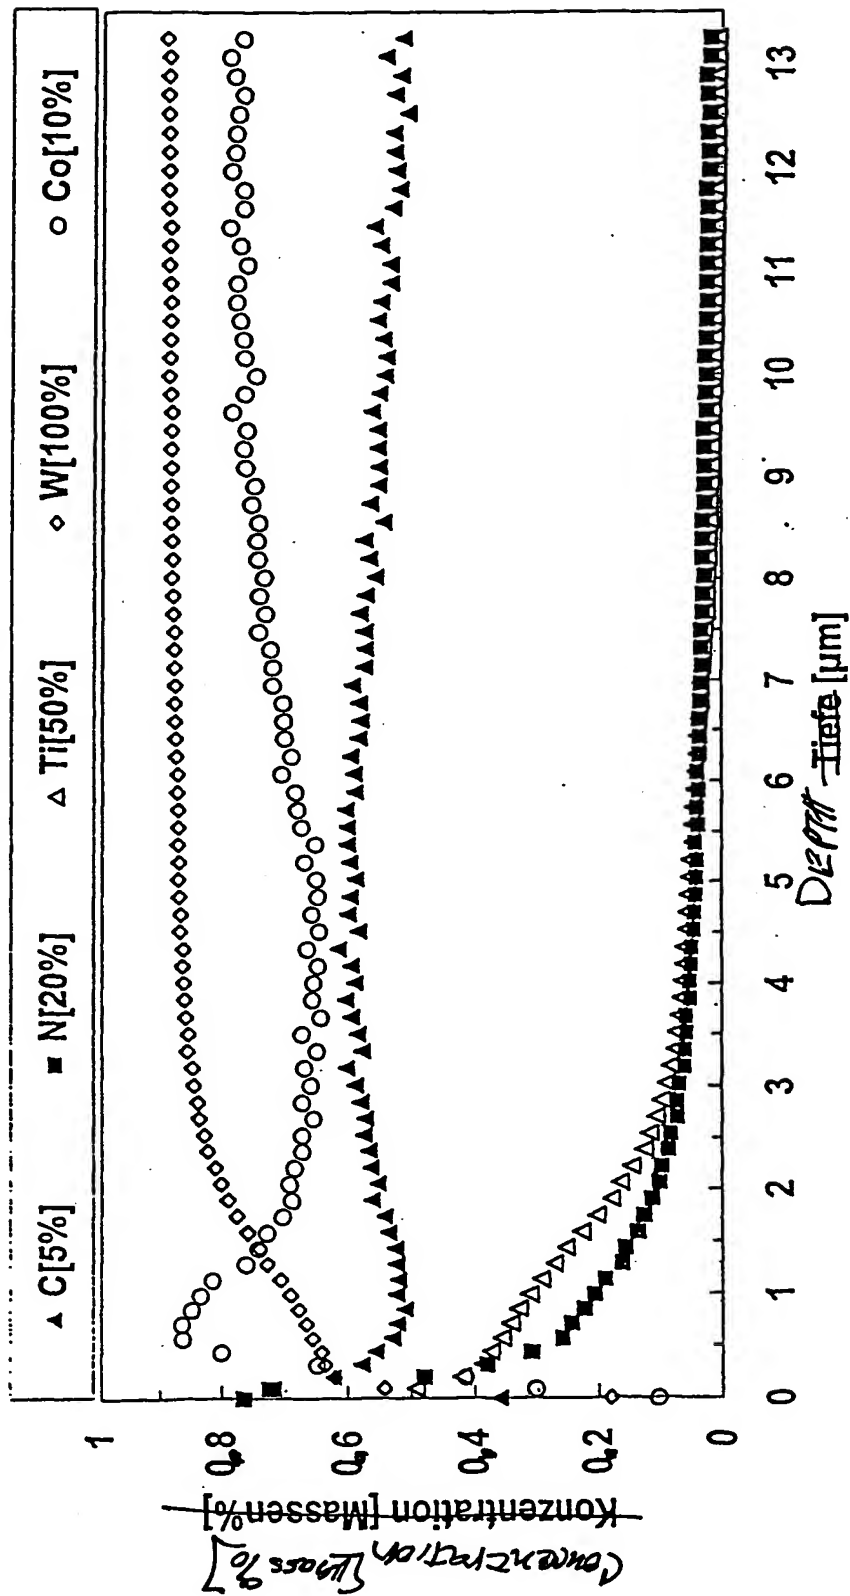

23091

3/8

FIG. 2 b

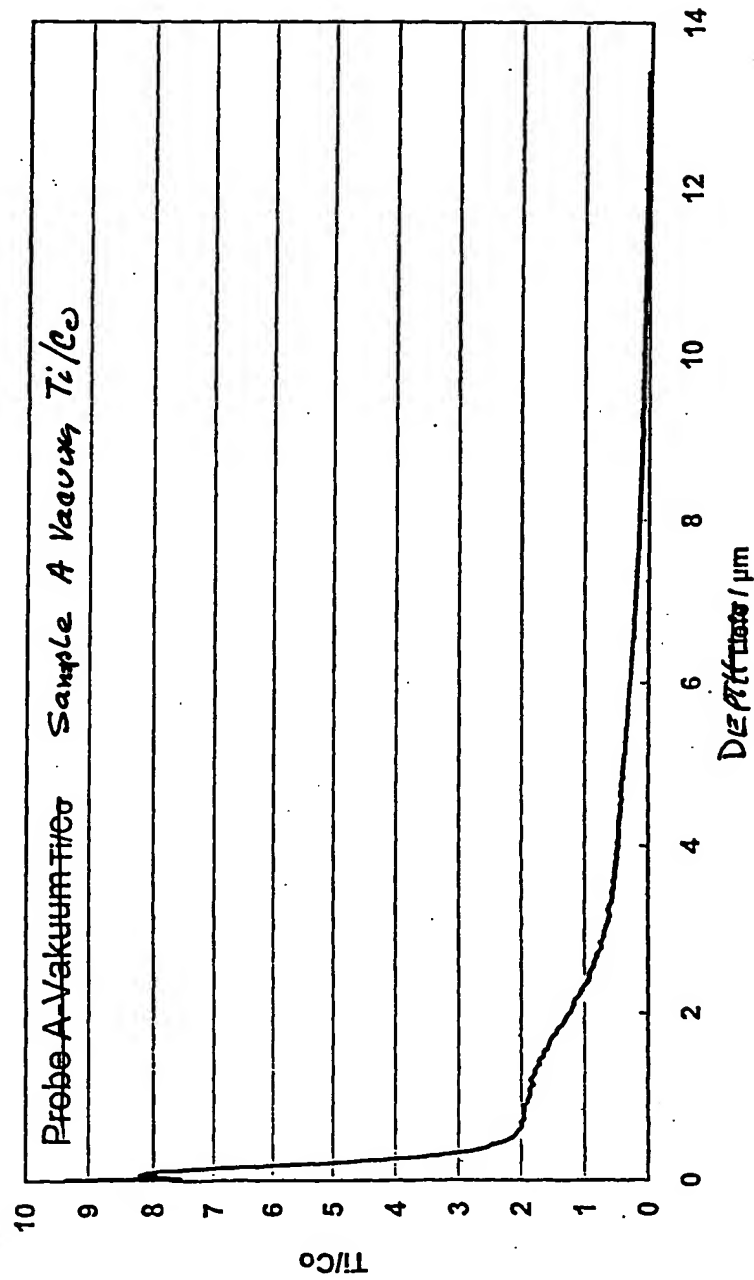


BEST AVAILABLE COPY

23091

4/8

FIG. 3a  
Tiefenprofil-Massentf. DEPTH PROFILE MASS %  
Probe C-Vakuum SAMPLE C - VACUUM

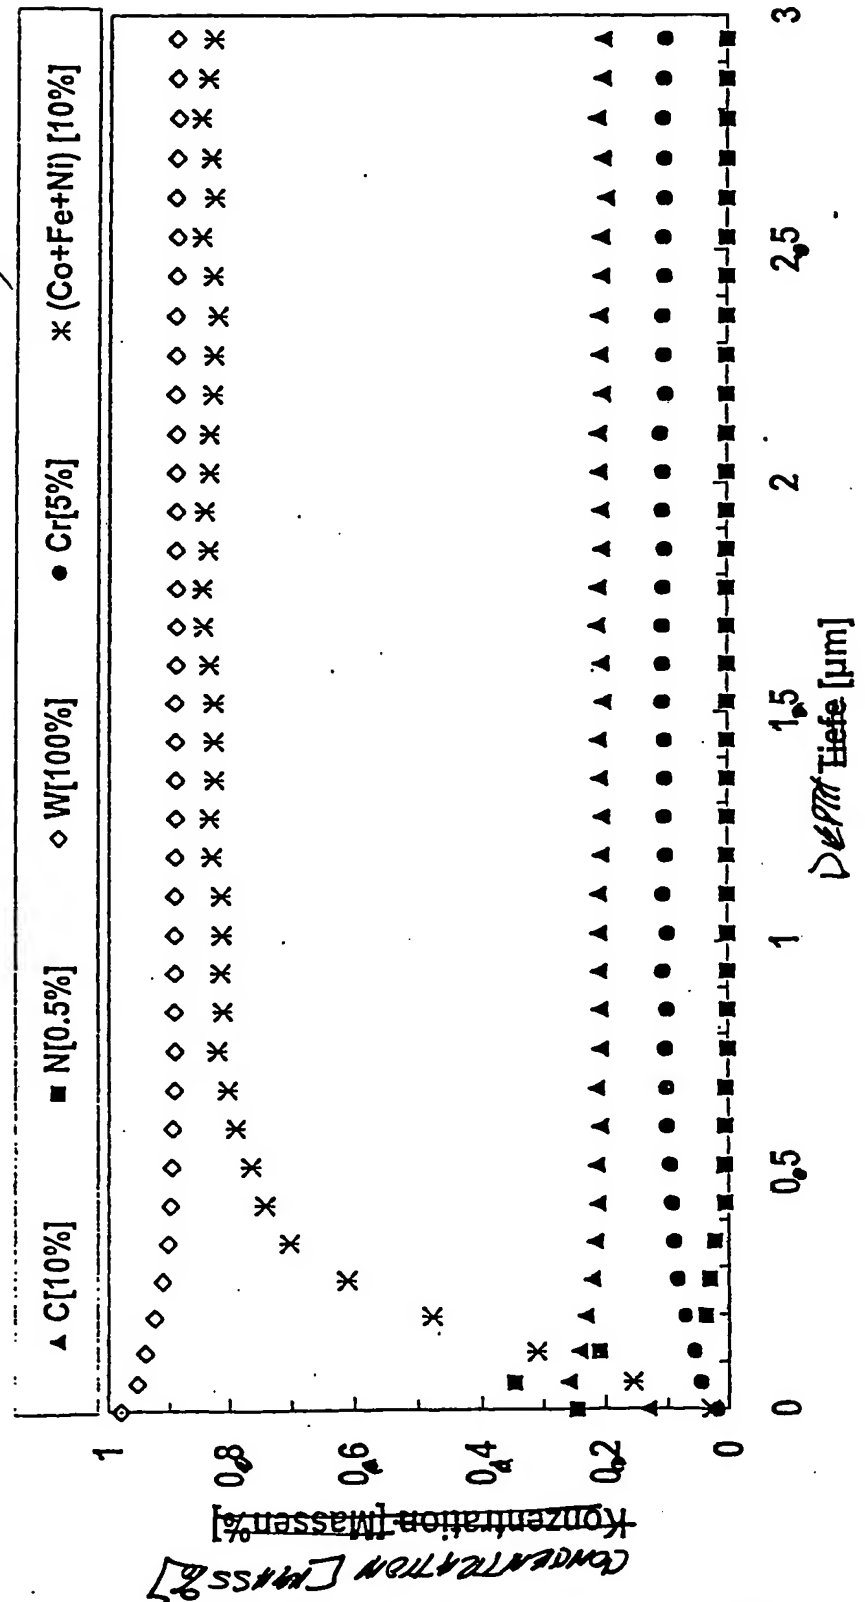


BEST AVAILABLE COPY

23091

5/8

FIG. 3b

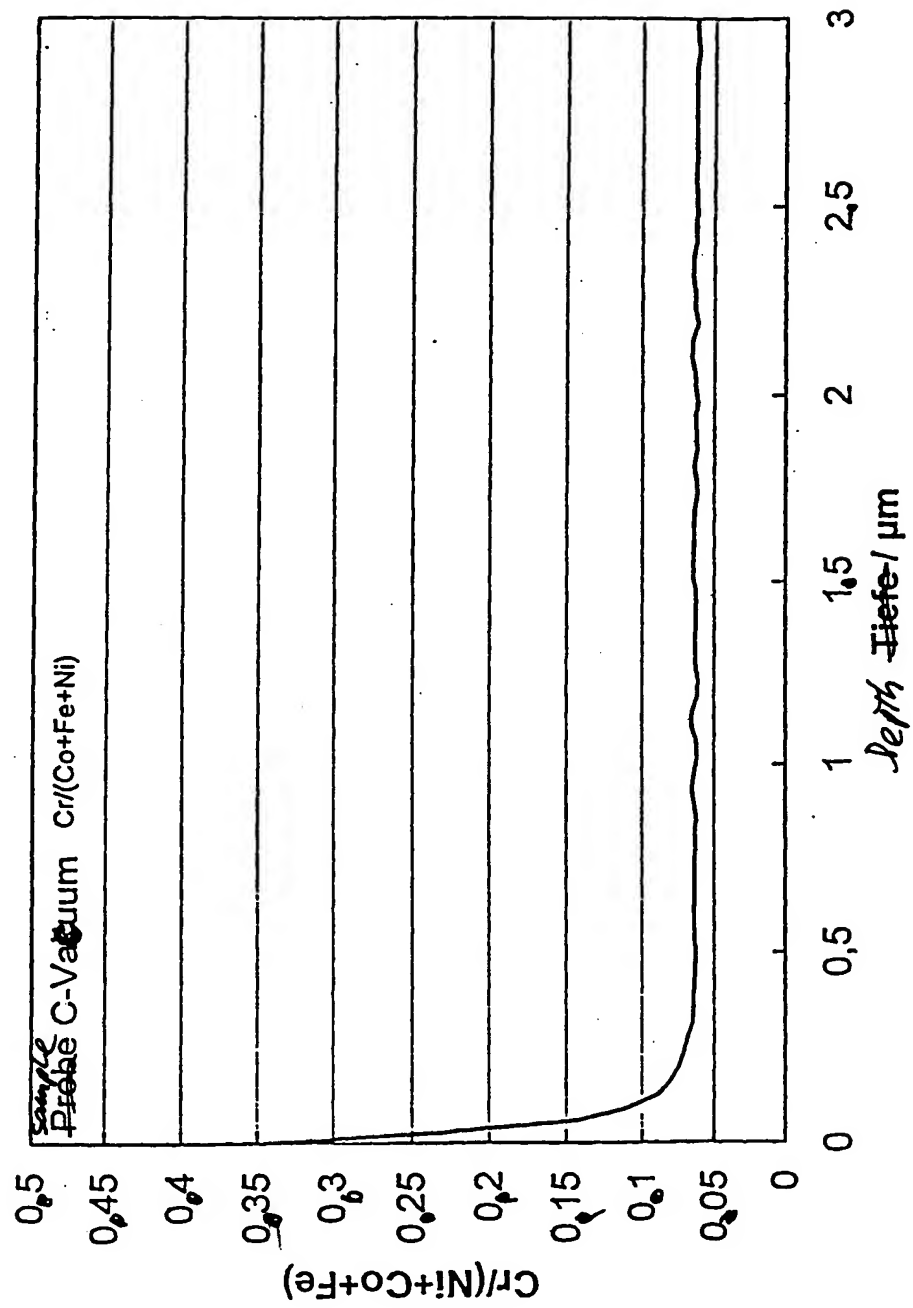

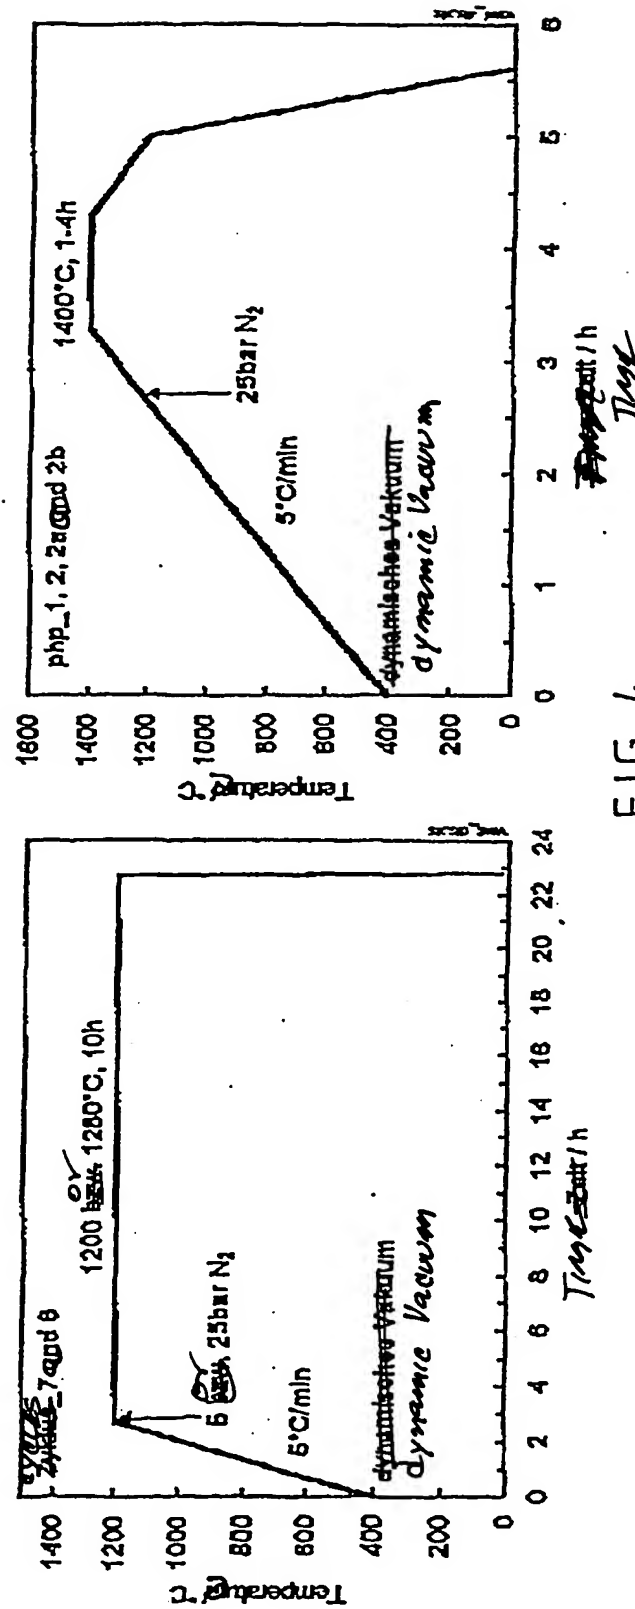


FIG. 4

23091

7/8


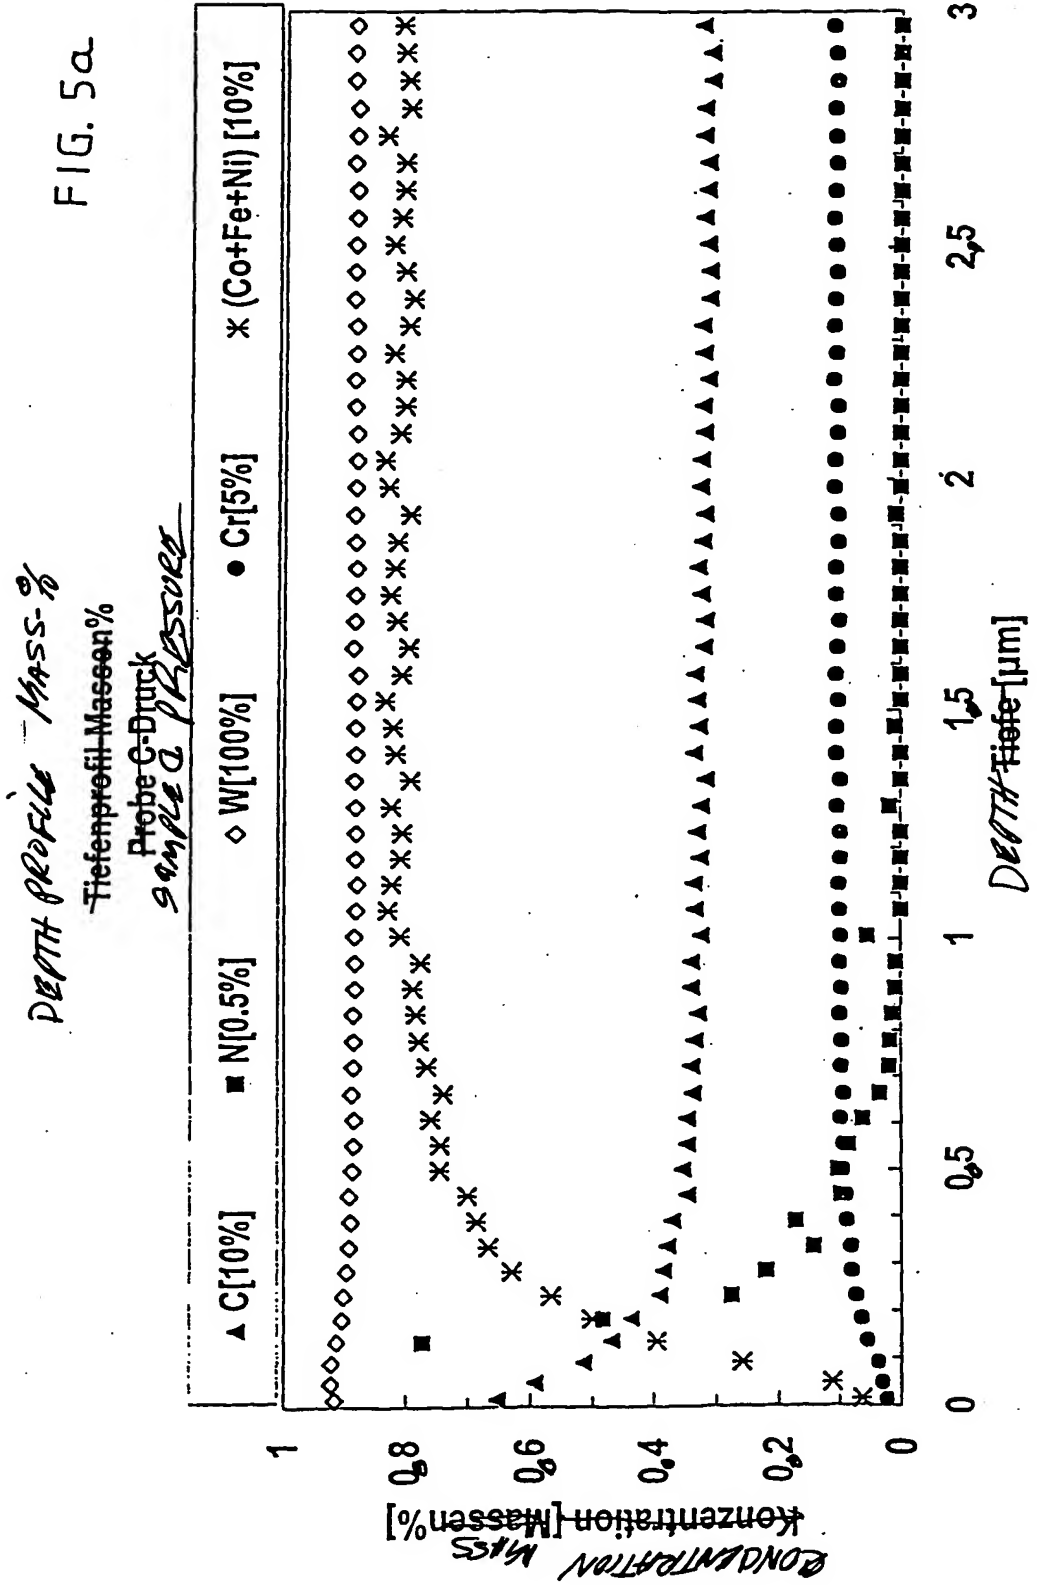


FIG. 5b

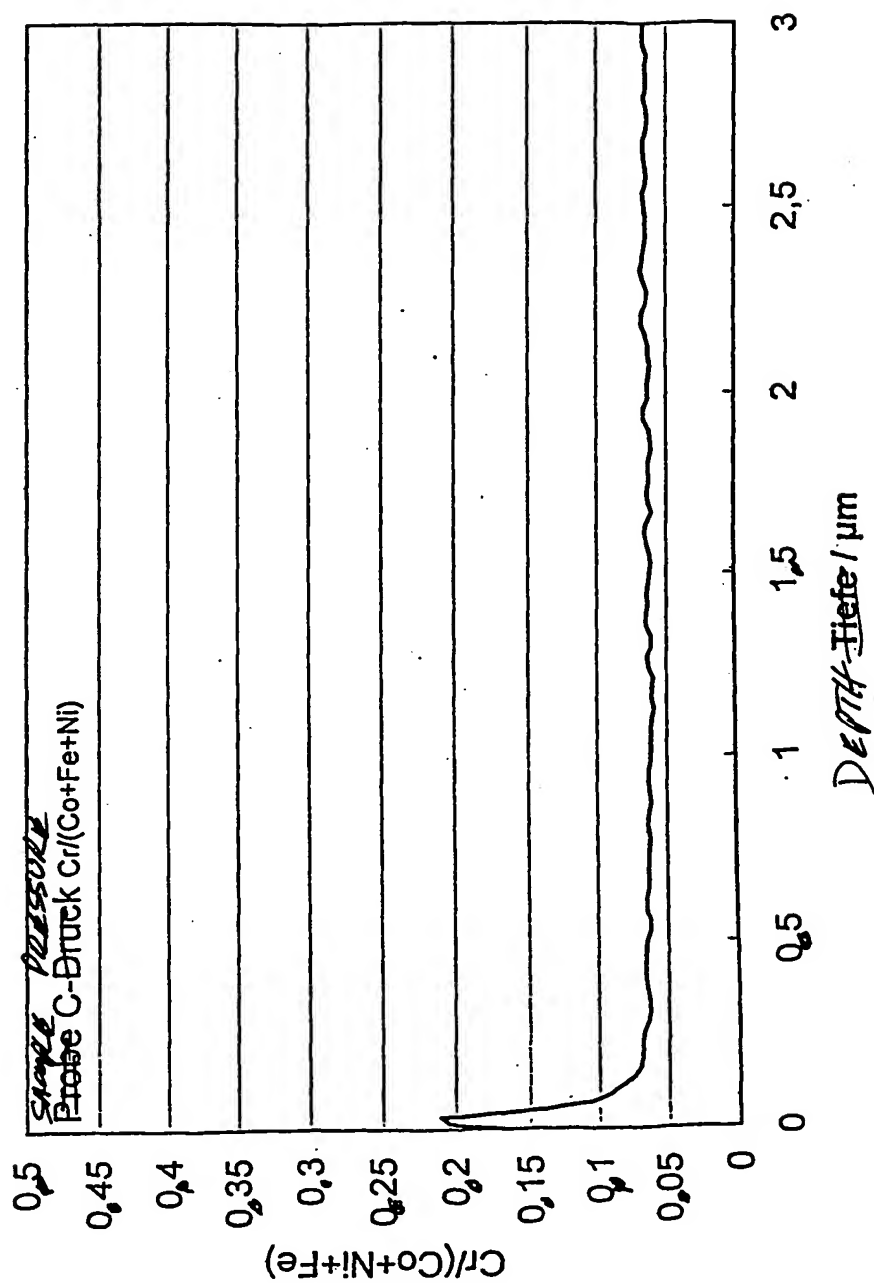

BEST AVAILABLE COPY